


FX 3000-IV: Exchange Display


- Open the top cover (two screws front left and right)
- Switch-off the instrument
- Disconnect the ribbon and power cable on the main pcb (see picture) be very careful with the ribbon cable connector.
- Exchange the display
- Reconnect ribbon and power cable

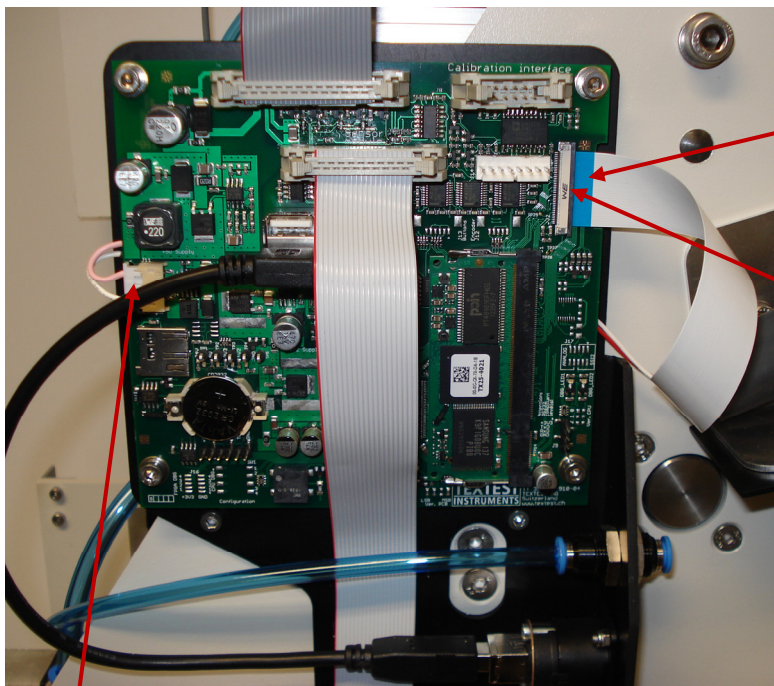

Connector ribbon cable

Be very careful with opening this ribbon cable connector.

Connector power cable

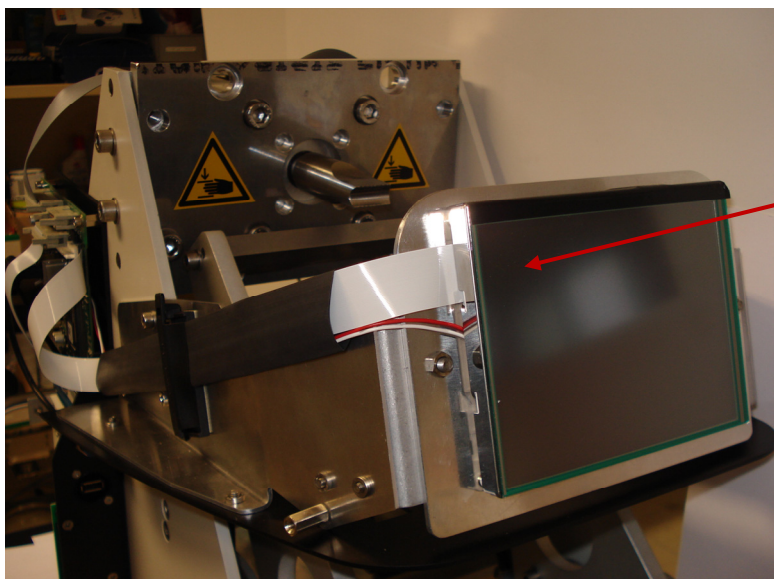

Display with cables