



FX 3300-IV: Instructions for replacement of TT 3300-4-930 Printed circuit board "Pressure sensors" 08/2020, NF


1. Disconnect the instrument from power line
2. Remove the front right panel

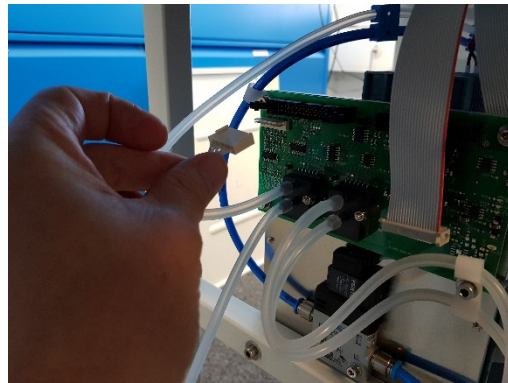


3. Disconnect all connectors

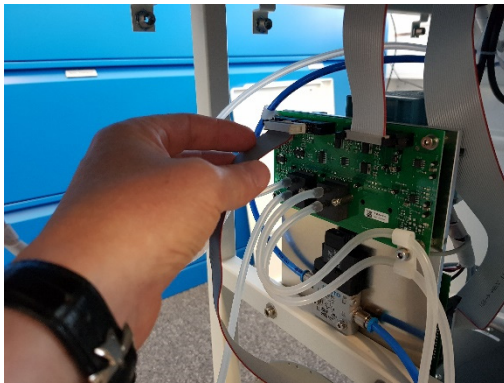


4. Using a marker pen, mark all 4 silicone hoses before disconnecting

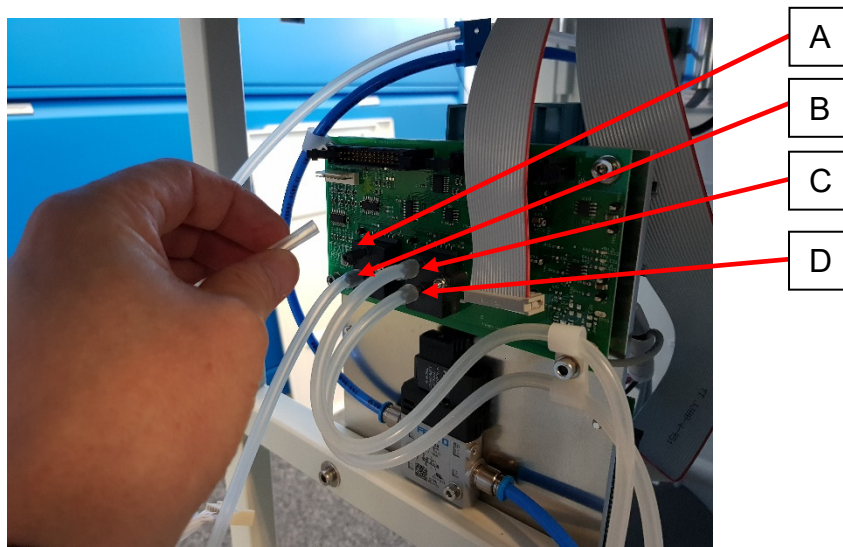


In case you missed to mark the hoses, the connections are as follows:

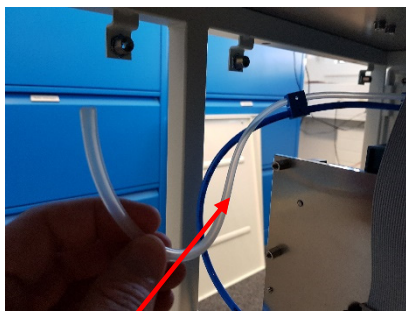


Hose A

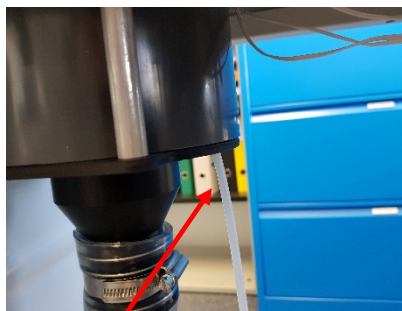

Hose B


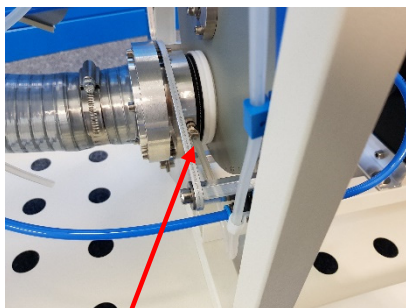


Hose C

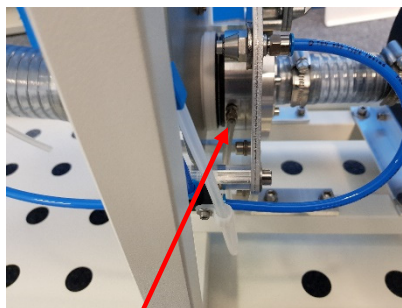

Hose D

5. Remove the mounting screws

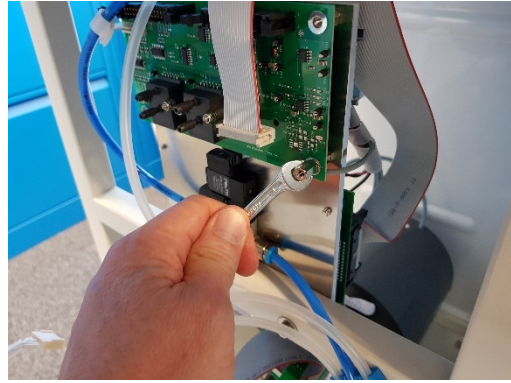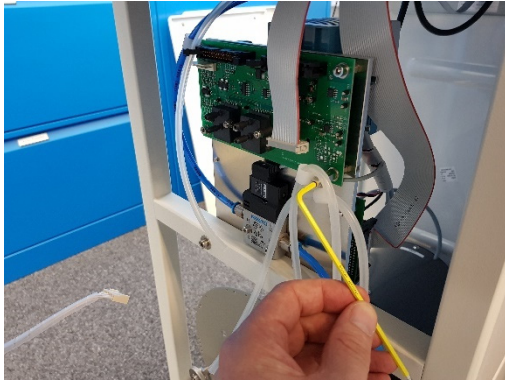

6. Remove the board and install the new board in reverse order

